

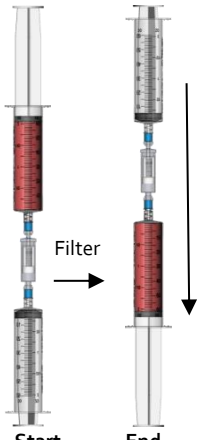


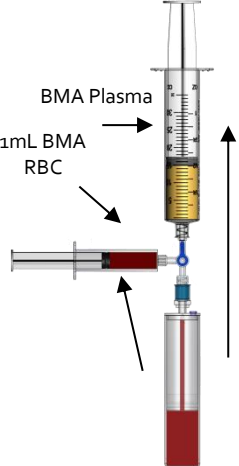
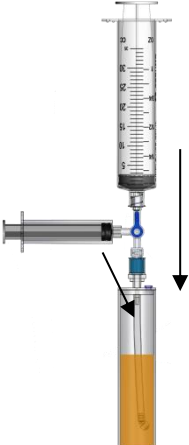


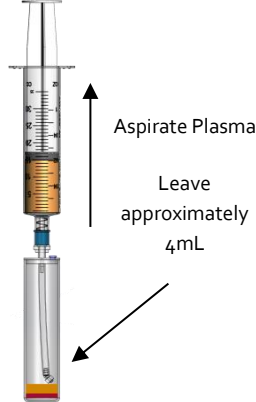
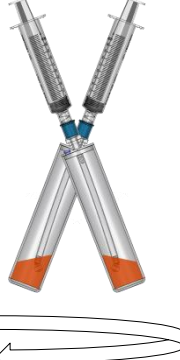
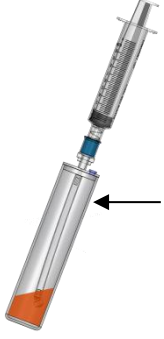
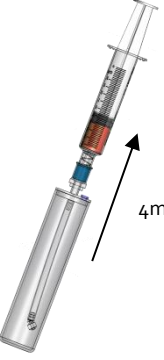


**BC30-PURE**

Note: Always swab self-sealing port with sterile alcohol prior to accessing with a sterile syringe

|  |   |  |   |
|--|---|--|---|
| <p>Step 1:</p>  <p>Using the filtered needle, draw 3mL of Citrate Anticoagulant into the 30mL Syringe.</p>                | <p>Step 2:</p>  <p>Draw 27mL BMA into the syringe, filling the syringe to 30mL.</p>                              | <p>Step 3:</p>  <p>Filter the 30mL of BMA into the 30mL syringe. Filter the BMA in the direction indicated on the filter.</p>  | <p>Step 4:</p>  <p>Inject anticoagulated &amp; filtered BMA into the Concentrating Device.</p> <p>Step 5:</p> <p>Counterbalance and process the Concentrating Device</p> <p><b>Executive Series Centrifuge</b><br/><b>1 minutes</b><br/><b>4200 RPM</b></p>  <p><b>Platinum Series Centrifuge</b><br/>Pre-Programmed Setting:<br/><b>PureBMC® SP Spin 1</b></p> |
| <p>Step 5:</p>  <p>Aspirate the plasma into the 30mL syringe. Then aspirate 1mL of red blood cells into 3mL syringe.</p> | <p>Step 6:</p>  <p>Transfer the plasma and RBC into the Concentrating Accessory.</p>                            | <p>Step 7:</p> <p>Counterbalance and process the Concentrating Device</p> <p><b>Executive Series Centrifuge</b><br/><b>5 minutes</b><br/><b>4200 RPM</b></p>  <p><b>Platinum Series Centrifuge</b><br/>Pre-Programmed Setting:<br/><b>PureBMC® SP Spin 2</b></p> | <p>Step 8:</p>  <p>Platelet buffycoat separates out at the bottom of the Concentrating Accessory.</p>   |
| <p>Step 9:</p>  <p>Aspirate plasma from the Concentrating Accessory. Leave 4mL of plasma.</p>                           | <p>Step 10:</p>  <p>Attach the 12mL syringe and swirl to resuspend the platelet buffycoat into the plasma.</p> | <p>Step 11:</p>  <p>Tilt to immerse Aspirating Pipe into PureBMC®</p>   | <p>Step 12:</p>  <p>Extract the PureBMC® PRP into the 12mL syringe.</p>  |