
## GSBMA-30 \*\*PLEASE DISCARD RED VENTED CAP FROM CONCENTRATION DEVICE BEFORE USE\*\*

Note: Always swab self-sealing port with sterile alcohol swab prio to accessing with a sterile syringe.

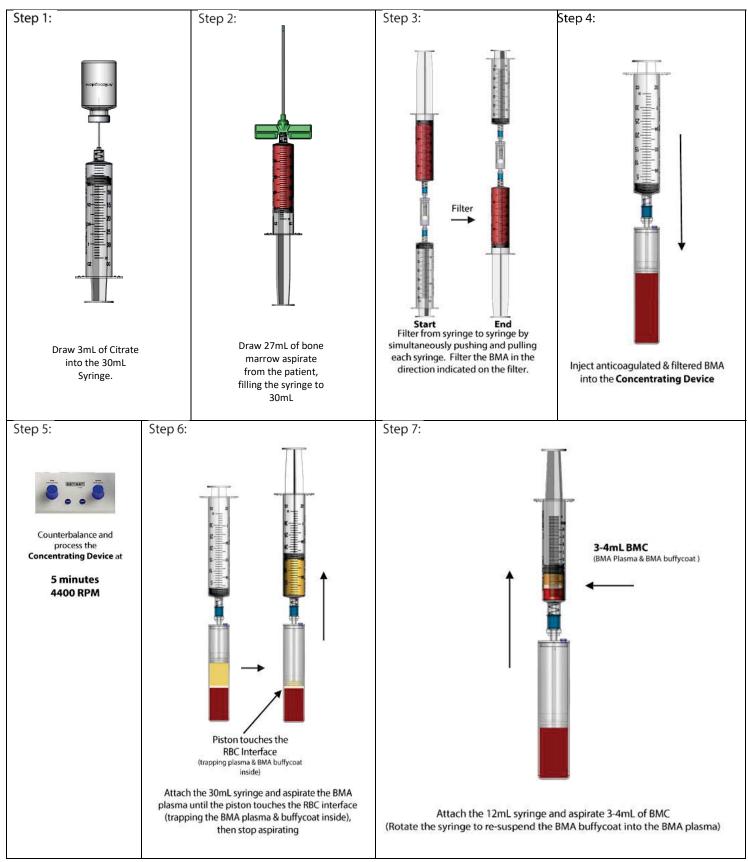

PL-42-36, REV. 8